

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat. No. : RP11095
 Lot. No. : E6319921G
 Time Processed : 2:24:11 PM
 Month-Day-Year Processed : 08/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

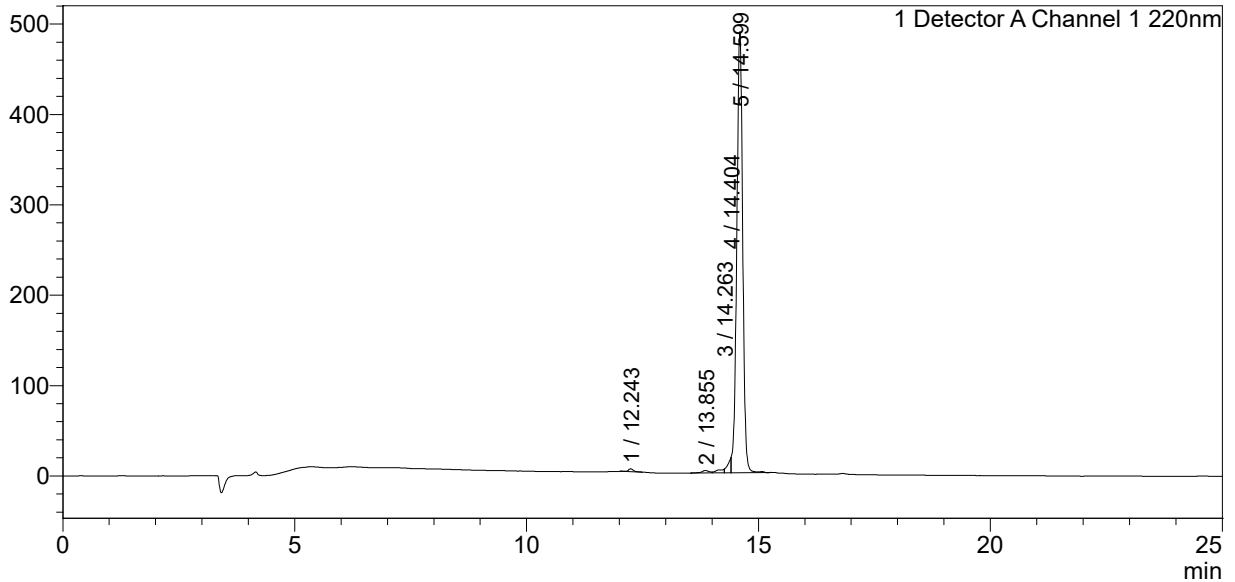

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.243	23737	3247	0.525
2	13.855	30974	2788	0.686
3	14.263	42609	3893	0.943
4	14.404	83954	15911	1.859
5	14.599	4336006	488166	95.987
Total		4517281	514005	100.000