

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP20527  
 Lot. No.: PE6231811  
 Time Processed :14:14:21  
 Month-Day-Year Processed :11/19/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

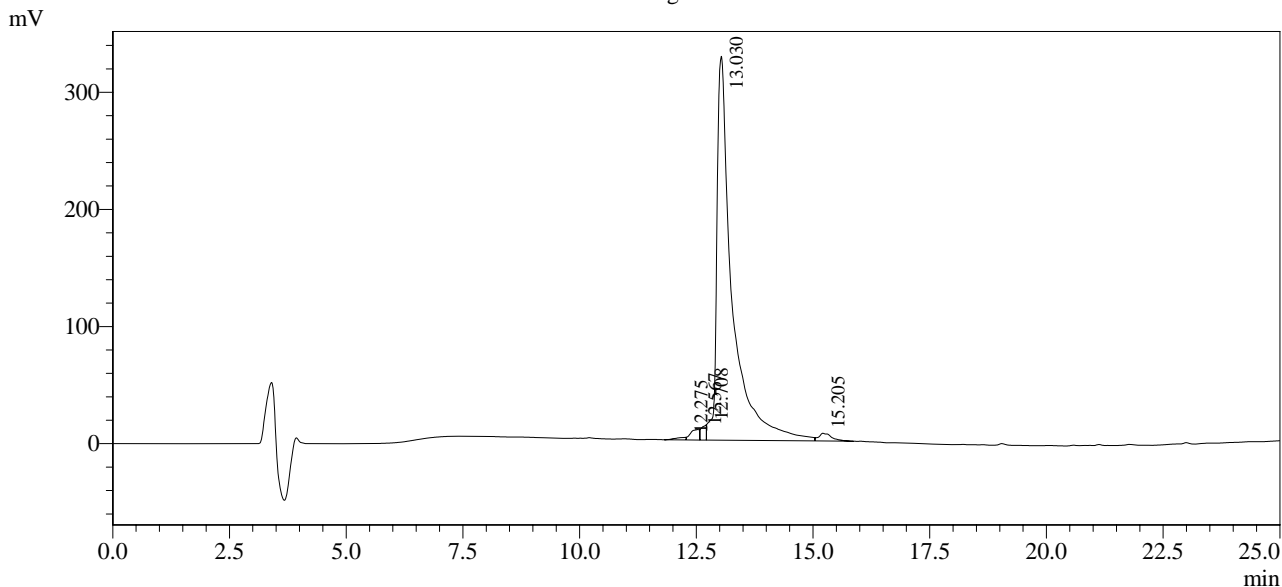

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.275	32577	2224	0.414
2	12.567	119172	8902	1.516
3	12.708	96118	12789	1.223
4	13.030	7483579	327794	95.218
5	15.205	127944	6586	1.628
Total		7859390	358295	100.000