

Sample Name :Calcitonin Gene Related Peptide (CGRP),rat
 Cat. No. :RP11095
 Lot. No. :PE5941902
 Time Processed : 9:26:09
 Month-Day-Year Processed : 02/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

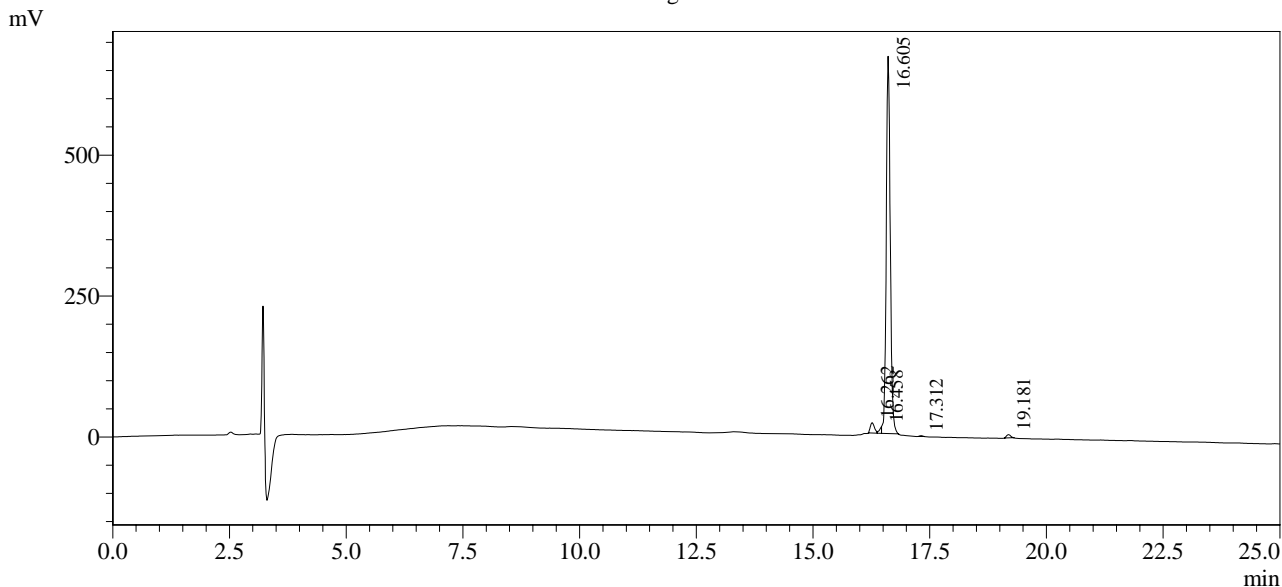

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.262	112468	18229	2.689
2	16.458	36341	11141	0.869
3	16.605	3994219	669132	95.513
4	17.312	4012	1038	0.096
5	19.181	34837	5769	0.833
Total		4181878	705309	100.000