

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), rat
 Cat No : RP11090
 Lot No : E8657921F
 Time Processed : 2:36:37
 Month-Day-Year Processed : 06/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

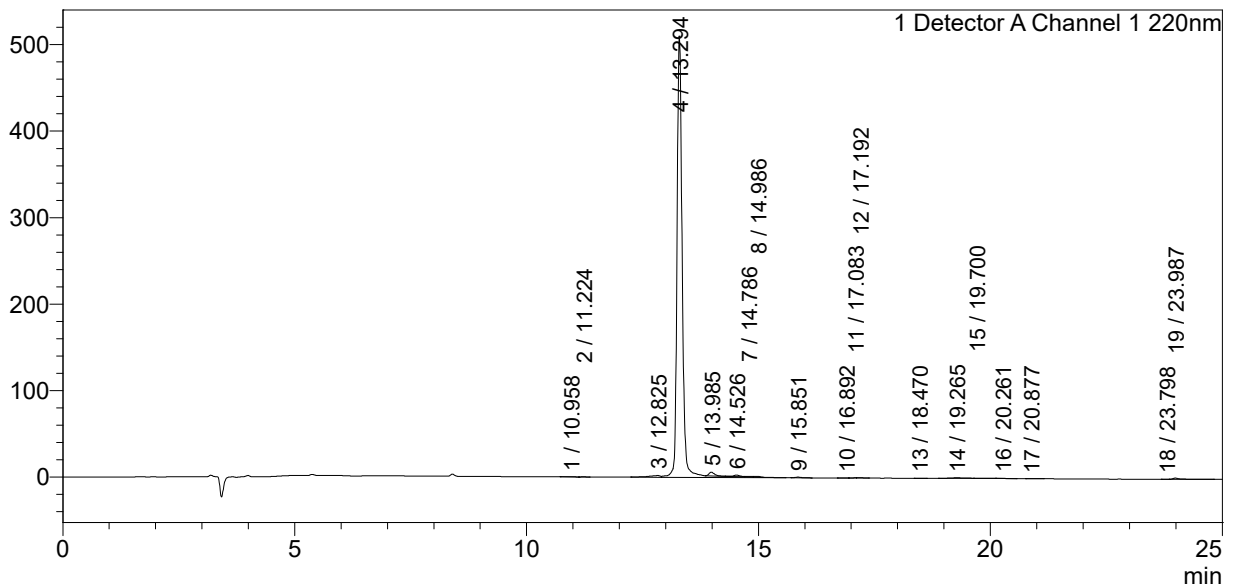

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.958	3661	351	0.087
2	11.224	1477	252	0.035
3	12.825	35590	2055	0.848
4	13.294	4027925	510702	95.954
5	13.985	38457	4449	0.916
6	14.526	17378	1670	0.414
7	14.786	5725	622	0.136
8	14.986	6324	766	0.151
9	15.851	6819	762	0.162
10	16.892	1135	123	0.027
11	17.083	2111	248	0.050
12	17.192	2996	333	0.071
13	18.470	1103	126	0.026
14	19.265	20895	739	0.498
15	19.700	4157	284	0.099
16	20.261	1329	103	0.032

Peak#	Ret. Time	Area	Height	Area%
17	20.877	1708	206	0.041
18	23.798	1069	159	0.025
19	23.987	17892	1457	0.426
Total		4197750	525406	100.000