

Sample Name : $\beta$ -Amyloid (1-42), human  
 Cat No. :RP20527  
 Lot No. :E2098720A  
 Time Processed :17:32:35  
 Month-Day-Year Processed :01/07/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

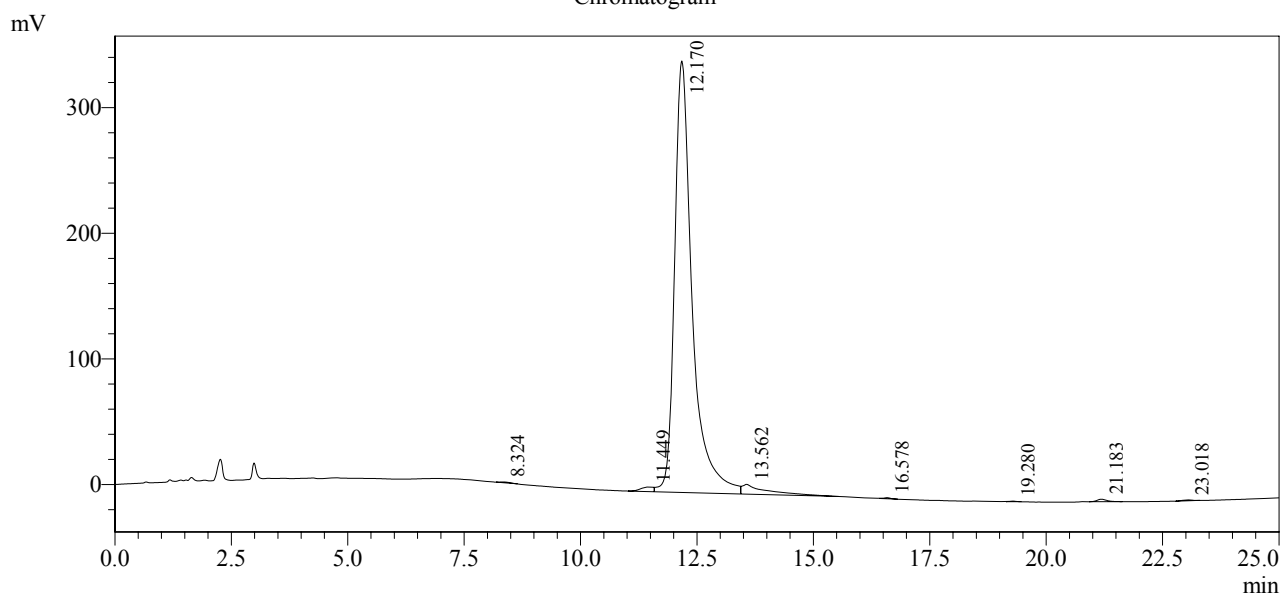

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.324	9246	545	0.098
2	11.449	68187	3530	0.723
3	12.170	9007817	343466	95.556
4	13.562	289870	7777	3.075
5	16.578	8204	862	0.087
6	19.280	3956	469	0.042
7	21.183	28930	1963	0.307
8	23.018	10495	748	0.111
Total		9426706	359360	100.000