

Sample Name : β -Amyloid (1-42), human
 Cat.No : RP10017
 Lot.No : E2304120G
 Time Processed: 15:53:02
 Year-Month-Day: 2020/7/8

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	10	
25.00	Pumps	Solvent B Conc.	100	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	10	
33.00	Pumps	Solvent B Conc.	10	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010015

<Chromatogram>

mV

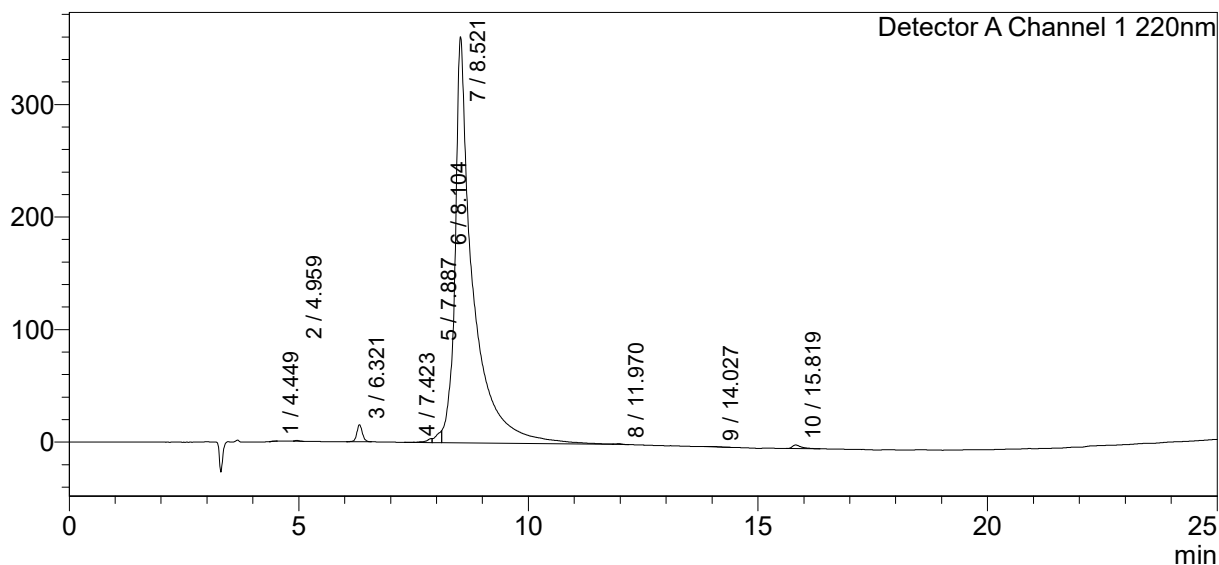

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.449	1661	309	0.017
2	4.959	3576	670	0.036
3	6.321	126485	15084	1.263
4	7.423	1258	161	0.013
5	7.887	32206	3619	0.322
6	8.104	85035	10212	0.849
7	8.521	9707818	360867	96.934
8	11.970	5249	658	0.052
9	14.027	6555	479	0.065
10	15.819	45079	3245	0.450
Total		10014923	395305	100.000