


Mass Spectrum

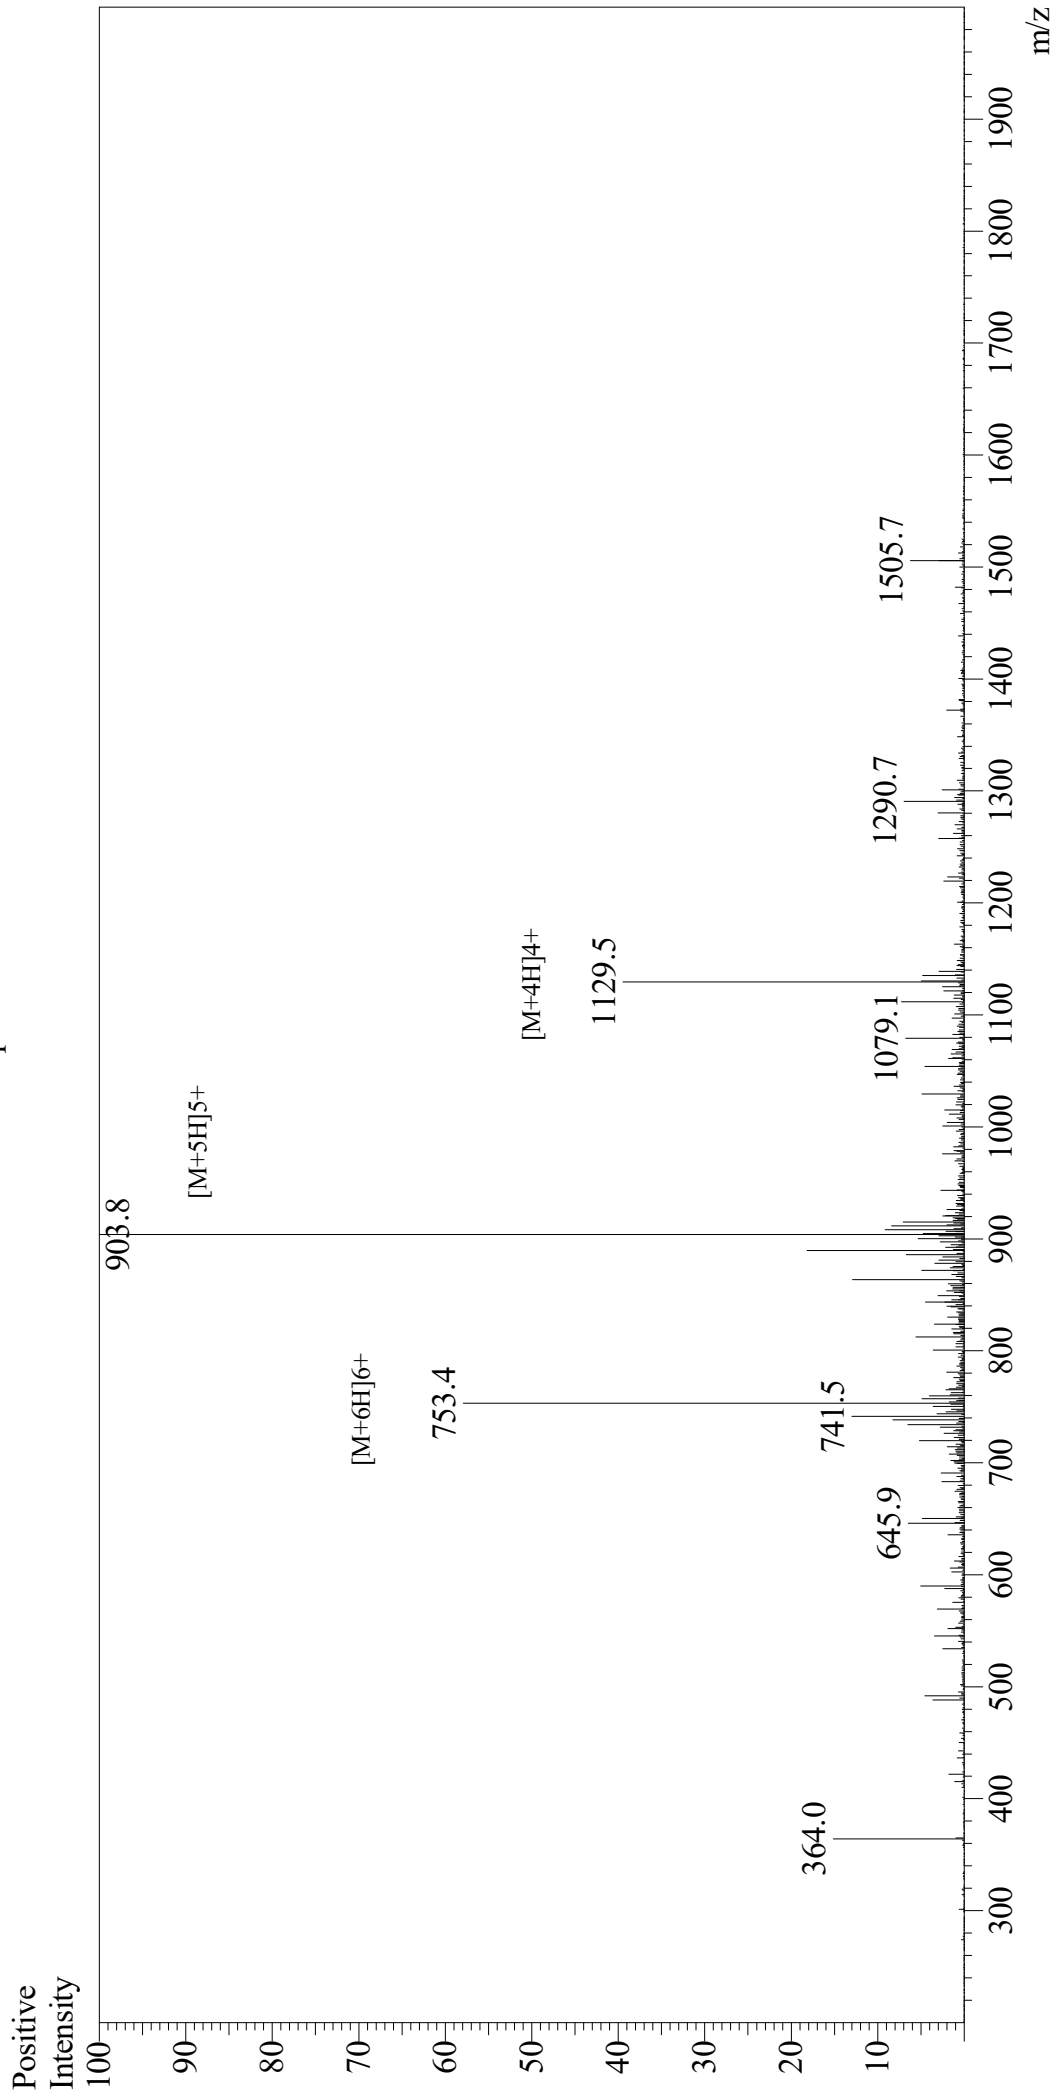

Sample Information
User : Gary
Month-Day Processed : 07/08/20
Time Processed : 05:42:02 PM
Injection Volume : 1
Sample Name : β -Amyloid (1-42), human
Cat No. : RP10017
Lot No. : E2304120G
Theoretical MW : 4514.10
Observed MW : 4514.0

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200