

Sample Name : Secretin, human
 Cat No : RP10249
 Lot No : E2664421E
 Time Processed : 18:39:49
 Month-Day-Year Processed : 05/07/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : SS-CM-0309

<Chromatogram>

mV

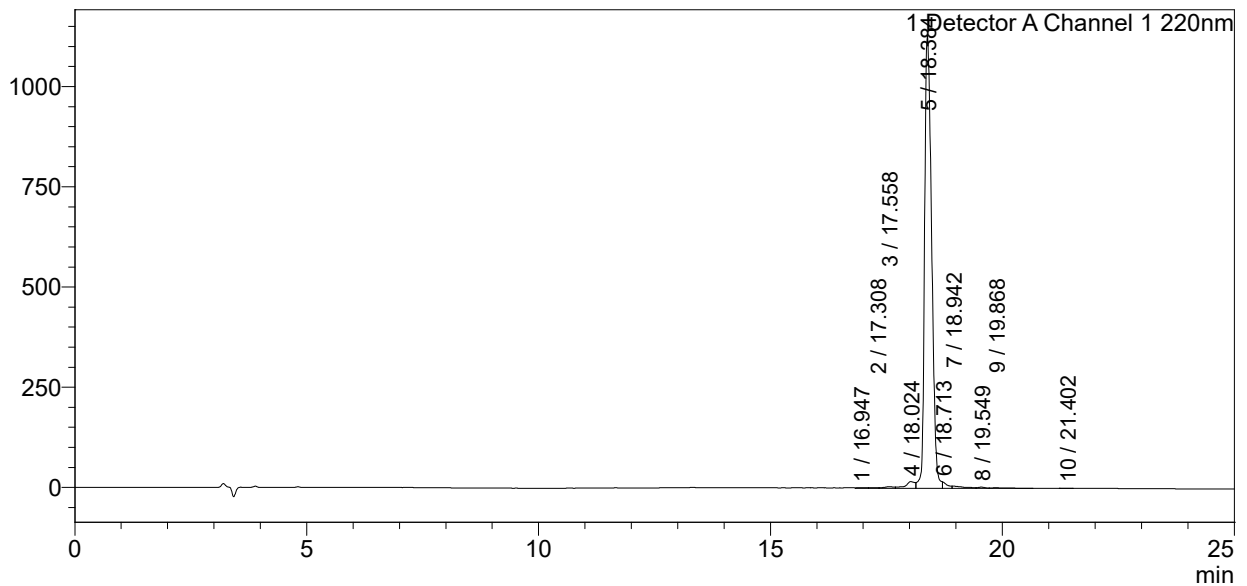

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.947	19927	1348	0.159
2	17.308	17582	1422	0.141
3	17.558	59338	4085	0.474
4	18.024	232857	16694	1.861
5	18.384	11923577	1129376	95.290
6	18.713	110601	16151	0.884
7	18.942	93442	5217	0.747
8	19.549	30059	2873	0.240
9	19.868	23728	1576	0.190
10	21.402	1881	151	0.015
Total		12512993	1178894	100.000