

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE6501905
 Time Processed :1:18:22
 Month-Day-Year Processed :05/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

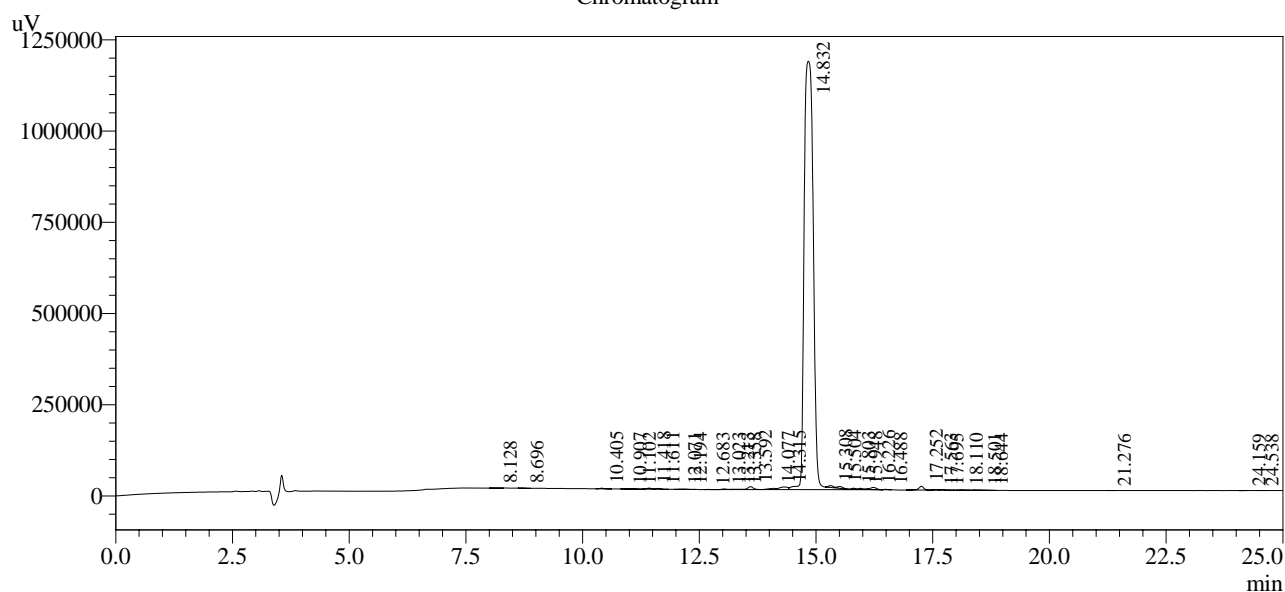

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.128	1973	198	0.012
2	8.696	2956	480	0.018
3	10.405	10452	1748	0.063
4	10.907	2704	366	0.016
5	11.102	1938	286	0.012
6	11.418	21859	2734	0.132
7	11.611	16615	2246	0.100
8	12.071	4751	673	0.029
9	12.194	7430	998	0.045
10	12.683	1669	299	0.010
11	13.023	14915	1913	0.090
12	13.213	11952	1188	0.072
13	13.358	6708	1044	0.040
14	13.592	70163	8200	0.423
15	14.077	40641	3684	0.245
16	14.315	93213	7315	0.563
17	14.832	15936404	1174315	96.181
18	15.308	41650	5186	0.251
19	15.504	42631	5191	0.257
20	15.803	18313	3067	0.111
21	15.948	18301	3017	0.110
22	16.226	63442	5976	0.383
23	16.488	6251	1179	0.038
24	17.252	81604	10573	0.493

Peak#	Ret. Time	Area	Height	Area %
25	17.563	10541	1669	0.064
26	17.695	14755	1667	0.089
27	18.110	10128	870	0.061
28	18.501	7481	1032	0.045
29	18.644	4546	617	0.027
30	21.276	1060	166	0.006
31	24.159	1056	120	0.006
32	24.538	1051	153	0.006
Total		16569155	1248172	100.000