

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No. : RP11095  
 Lot No. : PE6141901  
 Time Processed : 3:08:50  
 Month-Day-Year Processed : 02/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK12010012

<Chromatogram>

mV

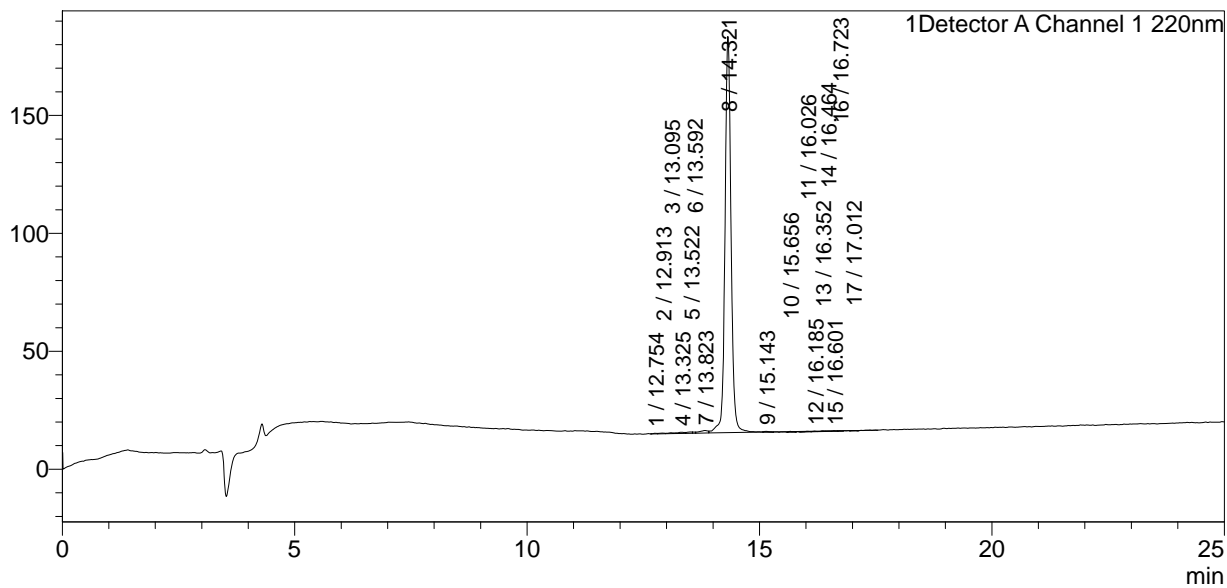

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.754	1466	281	0.095
2	12.913	2283	300	0.148
3	13.095	2407	340	0.156
4	13.325	5820	497	0.377
5	13.522	4511	575	0.292
6	13.592	1999	521	0.129
7	13.823	13627	1085	0.882
8	14.321	1497137	167955	96.917
9	15.143	2745	350	0.178
10	15.656	2151	410	0.139
11	16.026	1794	240	0.116
12	16.185	1231	225	0.080
13	16.352	1916	339	0.124
14	16.464	1324	230	0.086
15	16.601	1770	292	0.115

Peak#	Ret. Time	Area	Height	Area%
16	16.723	1179	195	0.076
17	17.012	1396	201	0.090
Total		1544756	174035	100.000