

Sample Name :Neuropeptide Y, human  
 Cat. No. : RP10492-0.5  
 Lot. No. :PE8151902  
 Time Processed :9:47:28  
 Month-Day-Year Processed :03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

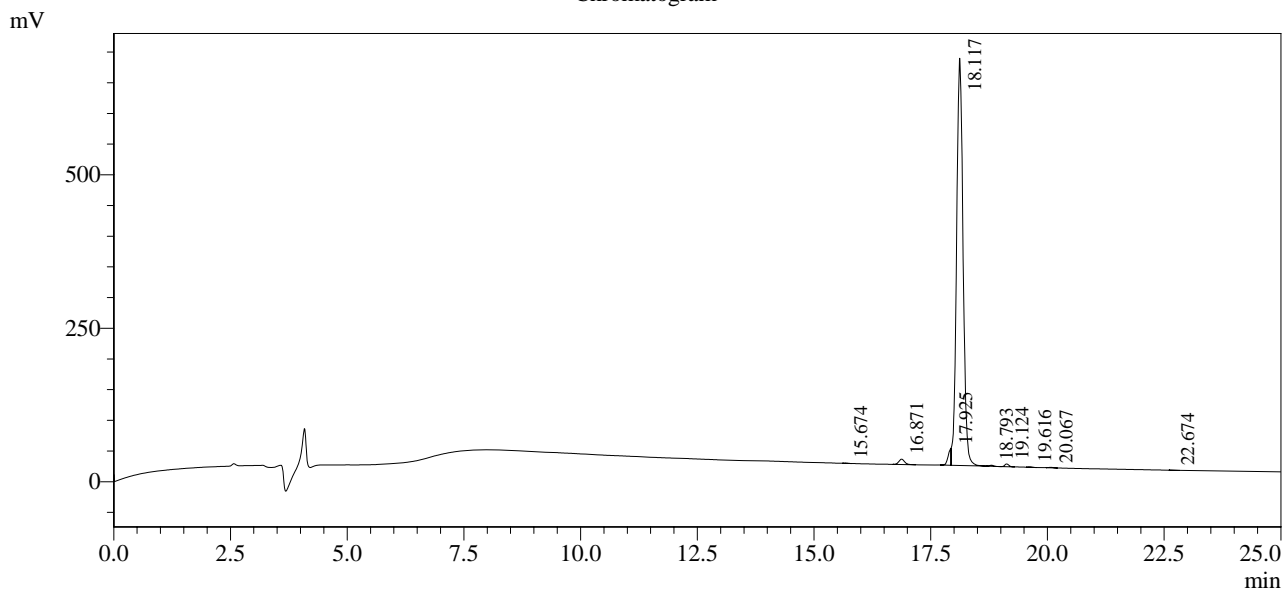

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.674	2047	367	0.031
2	16.871	74325	8696	1.112
3	17.925	117667	26726	1.760
4	18.117	6441523	663173	96.354
5	18.793	10183	1748	0.152
6	19.124	28213	4598	0.422
7	19.616	4387	765	0.066
8	20.067	5037	763	0.075
9	22.674	1919	303	0.029
Total		6685302	707140	100.000