

Sample Name:hgp100(25-33)  
 Cat. No. : RP20344  
 Lot. No. : E0629919H  
 Time Processed : 7:17:36  
 Month-Day-Year Processed : 08/15/2019  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

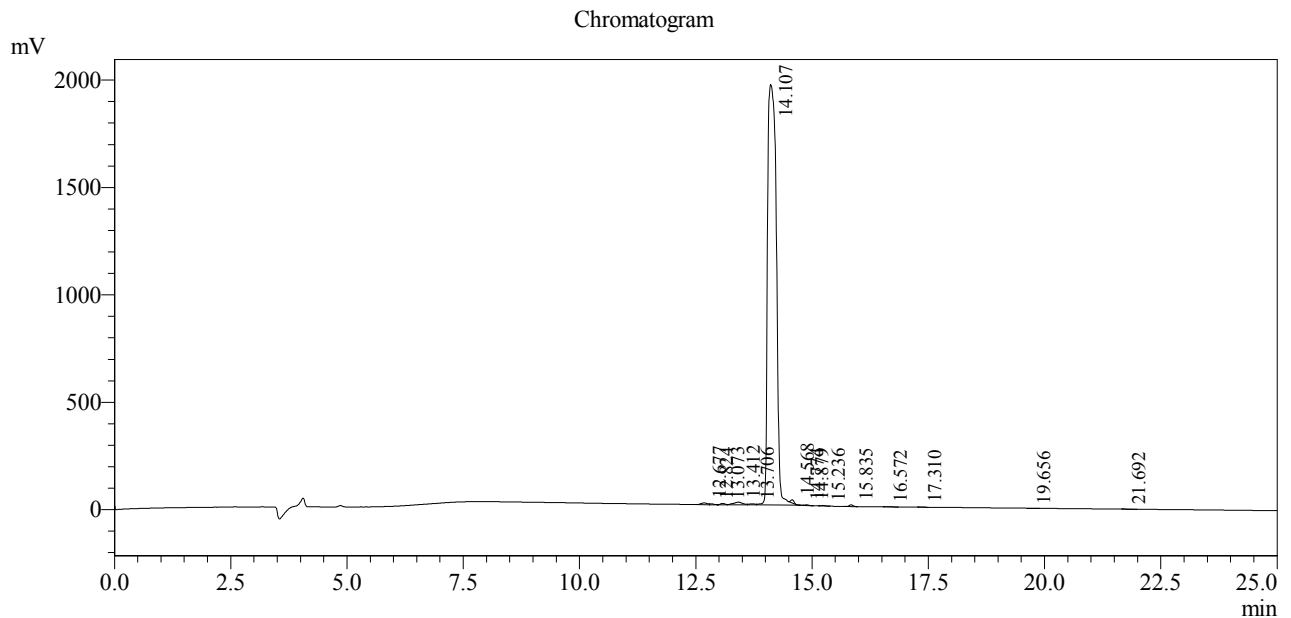

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.677	82015	8112	0.316
2	12.824	26587	4381	0.103
3	13.073	44251	6413	0.171
4	13.412	177247	12961	0.684
5	13.706	51899	5324	0.200
6	14.107	25383756	1957696	97.910
7	14.568	71773	15109	0.277
8	14.774	5354	1216	0.021
9	14.879	18314	3165	0.071
10	15.236	13662	2277	0.053
11	15.835	42842	7940	0.165
12	16.572	2853	205	0.011
13	17.310	1201	132	0.005
14	19.656	1285	67	0.005
15	21.692	2601	109	0.010
Total		25925641	2025107	100.000