

Sample Name : [Nle4, D-Phe7]- α -MSH, amide
 Cat. No. : RP10658
 Lot. No. : PE5261610

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

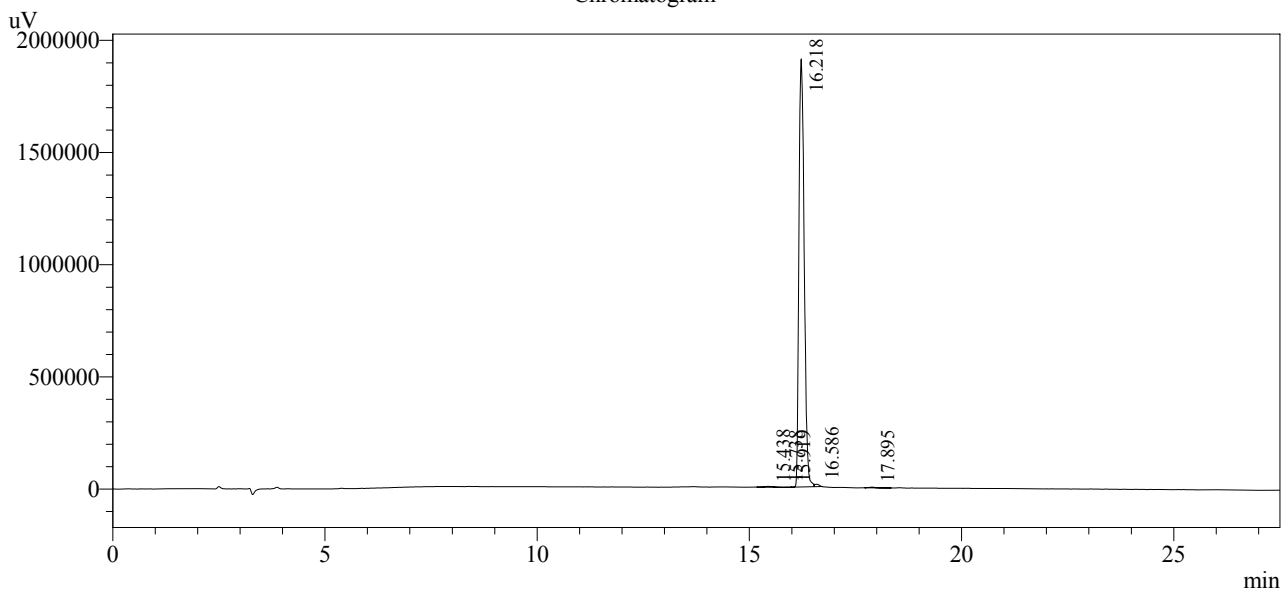

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.438	59239	3628	0.354
2	15.738	2649	1003	0.016
3	15.919	2592	552	0.015
4	16.218	16567345	1908308	99.053
5	16.586	77102	10338	0.461
6	17.895	16735	3169	0.100
Total		16725662	1926997	100.000