

Sample Name : Glucagon (1-29), Human
 Cat. No. : RP10772
 Lot. No. : E1461519H
 Time Processed : 12:40:38
 Month-Day-Year Processed : 08/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

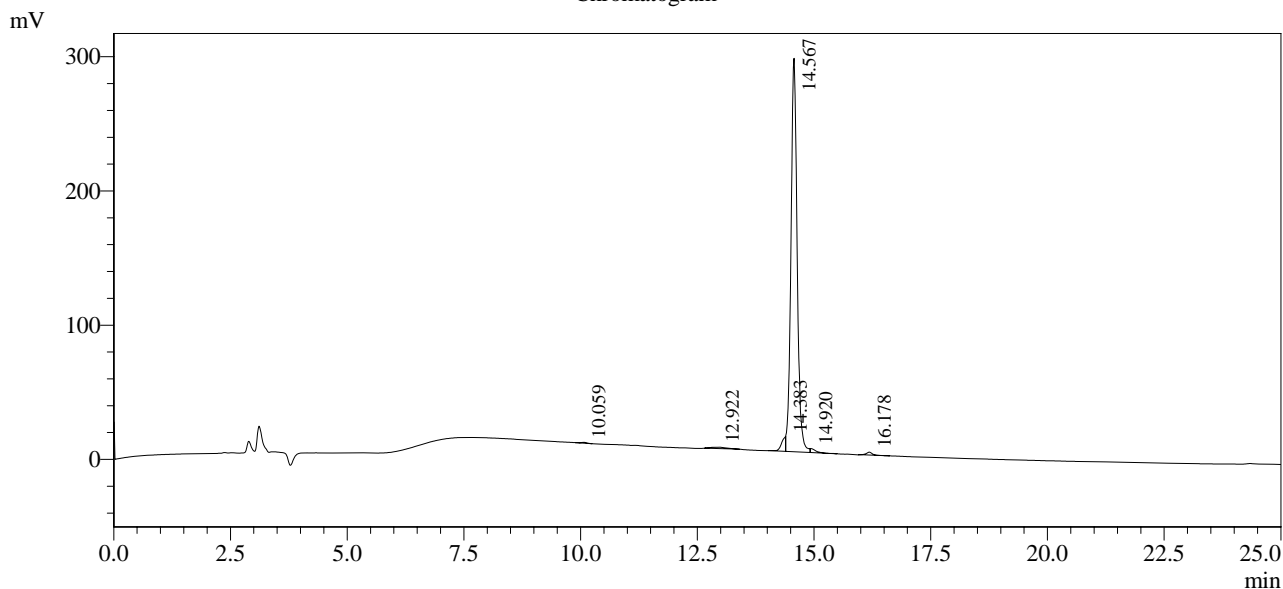

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.059	4545	609	0.160
2	12.922	23127	948	0.816
3	14.383	65308	10715	2.305
4	14.567	2700197	293201	95.289
5	14.920	23660	2925	0.835
6	16.178	16846	2061	0.594
Total		2833683	310458	100.000