

Sample Name : LH-RH, human, LH-RH
 Cat. No. : RP11937
 Lot. No. : E4895519I
 Time Processed :12:54:52
 Month-Day-Year Processed :09/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

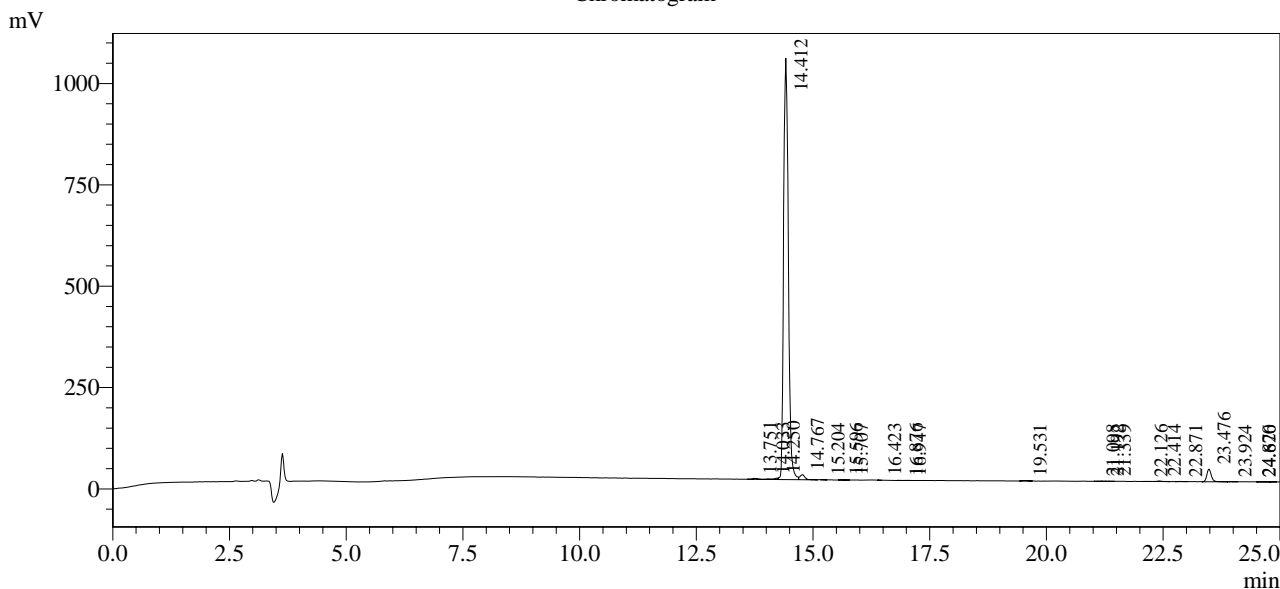

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.751	16032	2041	0.207
2	14.033	6251	1061	0.081
3	14.250	18495	3835	0.239
4	14.412	7364267	1039272	95.091
5	14.767	91152	12507	1.177
6	15.204	3049	540	0.039
7	15.596	1739	305	0.022
8	15.707	1022	292	0.013
9	16.423	1197	304	0.015
10	16.876	1401	310	0.018
11	16.947	2211	305	0.029
12	19.531	5446	876	0.070
13	21.098	1768	359	0.023
14	21.192	1780	389	0.023
15	21.339	2491	362	0.032
16	22.126	1153	206	0.015
17	22.414	10965	1348	0.142
18	22.871	3108	421	0.040
19	23.476	205059	30951	2.648
20	23.924	1425	204	0.018
21	24.670	2579	336	0.033
22	24.826	1828	367	0.024
Total		7744417	1096592	100.000