

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. : RP21087
 Lot No. : E7331821C
 Time Processed :9:07:39 PM
 Month-Day-Year Processed :03/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

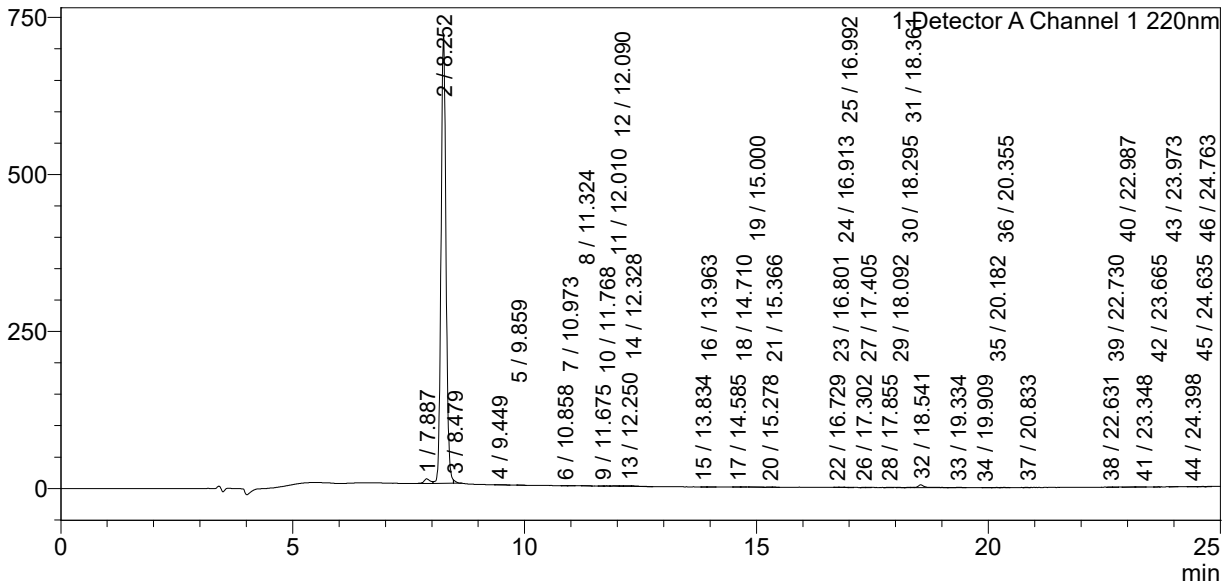

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.887	65117	7269	1.176
2	8.252	5319753	716203	96.069
3	8.479	15948	4697	0.288
4	9.449	3879	367	0.070
5	9.859	1173	151	0.021
6	10.858	1164	245	0.021
7	10.973	1066	196	0.019
8	11.324	2628	289	0.047
9	11.675	1044	238	0.019
10	11.768	2091	343	0.038
11	12.010	7210	802	0.130
12	12.090	4796	960	0.087
13	12.250	9326	985	0.168
14	12.328	12427	1125	0.224

Peak#	Ret. Time	Area	Height	Area%
15	13.834	1254	211	0.023
16	13.963	1060	174	0.019
17	14.585	1353	197	0.024
18	14.710	1899	316	0.034
19	15.000	4816	473	0.087
20	15.278	1318	182	0.024
21	15.366	1038	225	0.019
22	16.729	1074	221	0.019
23	16.801	1338	224	0.024
24	16.913	1105	219	0.020
25	16.992	1440	225	0.026
26	17.302	1220	231	0.022
27	17.405	1373	221	0.025
28	17.855	1573	182	0.028
29	18.092	1255	192	0.023
30	18.295	1500	298	0.027
31	18.361	1441	380	0.026
32	18.541	40881	4457	0.738
33	19.334	2639	246	0.048
34	19.909	1766	194	0.032
35	20.182	1538	228	0.028
36	20.355	2220	223	0.040
37	20.833	1479	245	0.027
38	22.631	1278	238	0.023
39	22.730	1330	214	0.024
40	22.987	2078	208	0.038
41	23.348	1220	156	0.022
42	23.665	1185	184	0.021
43	23.973	1817	228	0.033
44	24.398	2001	208	0.036
45	24.635	1225	160	0.022
46	24.763	1120	226	0.020
Total		5537457	745454	100.000