

Sample Name : MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No: RP21087
 Lot No : E4936320L
 Time Processed :1:55:40 PM
 Month-Day-Year Processed :12/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

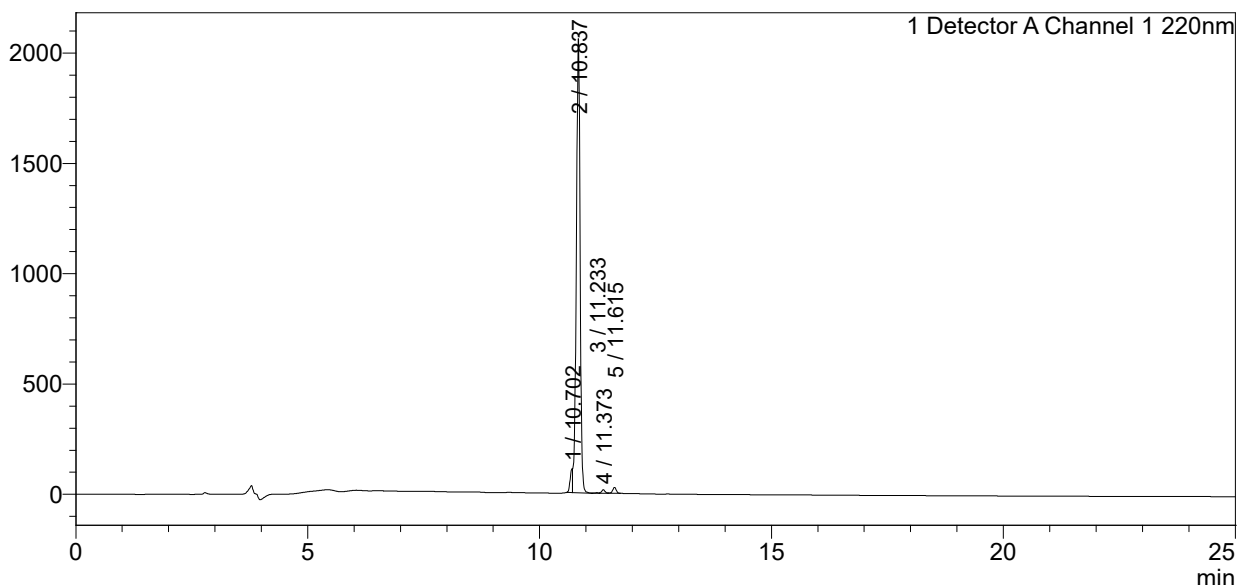

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.702	375613	107998	3.037
2	10.837	11759884	2058504	95.077
3	11.233	11814	2065	0.096
4	11.373	79033	15903	0.639
5	11.615	142490	26705	1.152
Total		12368834	2211176	100.000