

Sample Name : $\beta$ -Amyloid (25-35)  
 Cat No. :RP10008  
 Lot No. :E2684021A  
 Time Processed :22:52:33  
 Month-Day-Year Processed :01/06/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

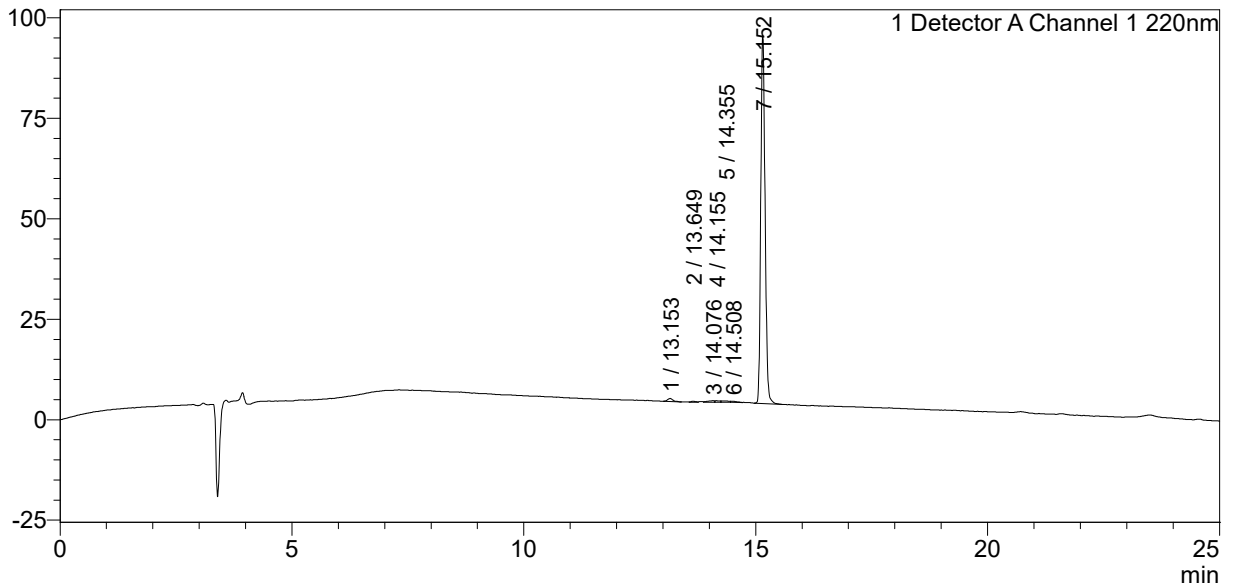

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.153	6197	745	1.008
2	13.649	1612	220	0.262
3	14.076	4009	385	0.652
4	14.155	2858	387	0.465
5	14.355	4174	387	0.679
6	14.508	2515	302	0.409
7	15.152	593378	91575	96.525
Total		614743	94002	100.000