

Sample Name : Chemerin-9 (149-157)  
 Cat. No. : RP20248  
 Lot. No. : PE2941901  
 Time Processed :19:15:13  
 Month-Day-Year Processed :02/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

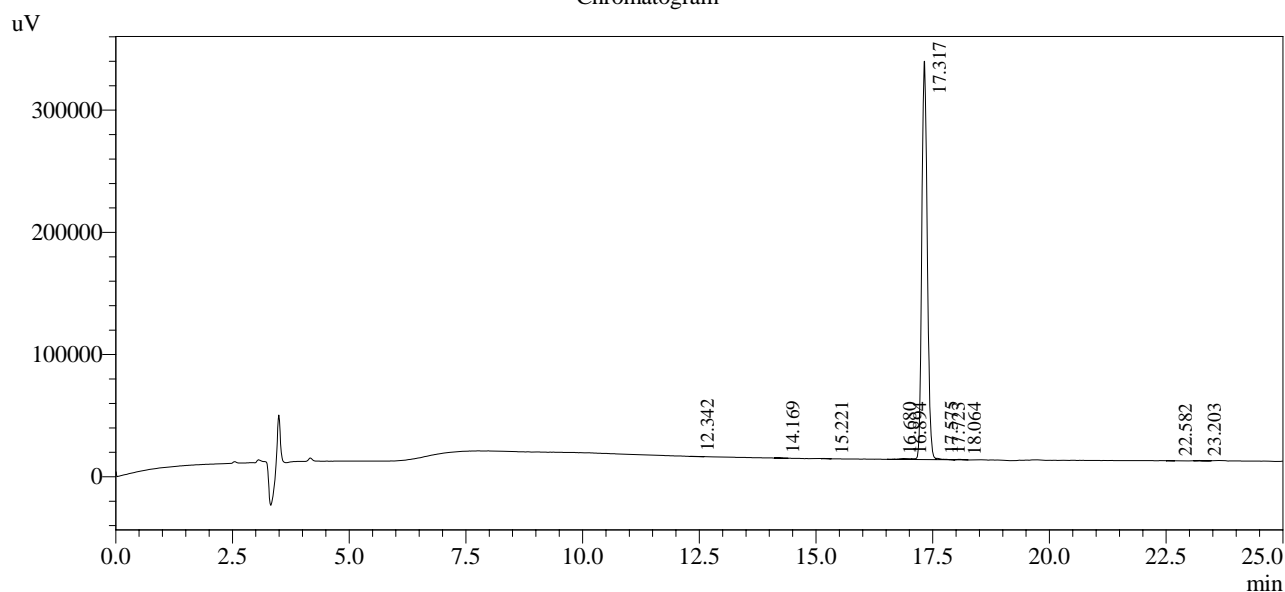

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.342	1162	109	0.043
2	14.169	1055	127	0.039
3	15.221	2200	404	0.081
4	16.680	1660	295	0.061
5	16.894	12450	819	0.460
6	17.317	2673015	326008	98.737
7	17.575	6286	1113	0.232
8	17.723	2859	380	0.106
9	18.064	2932	415	0.108
10	22.582	1018	174	0.038
11	23.203	2559	320	0.095
Total		2707194	330164	100.000