

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide

Cat No. : RP21087

Lot No. : E2230620D

Time Processed: 7:40:52 PM

Month-Day-Year Processed :04/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010324

<Chromatogram>

mV

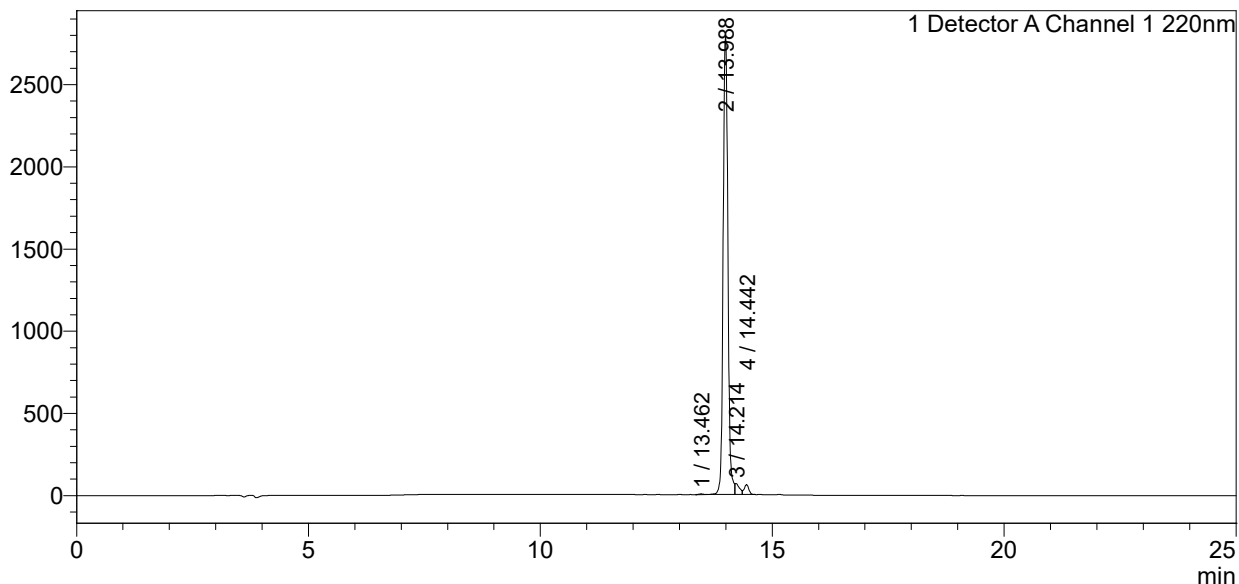

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.462	47249	4130	0.226
2	13.988	20033074	2786493	95.621
3	14.214	446868	66368	2.133
4	14.442	423272	60060	2.020
Total		20950463	2917052	100.000