


Mass Spectrum

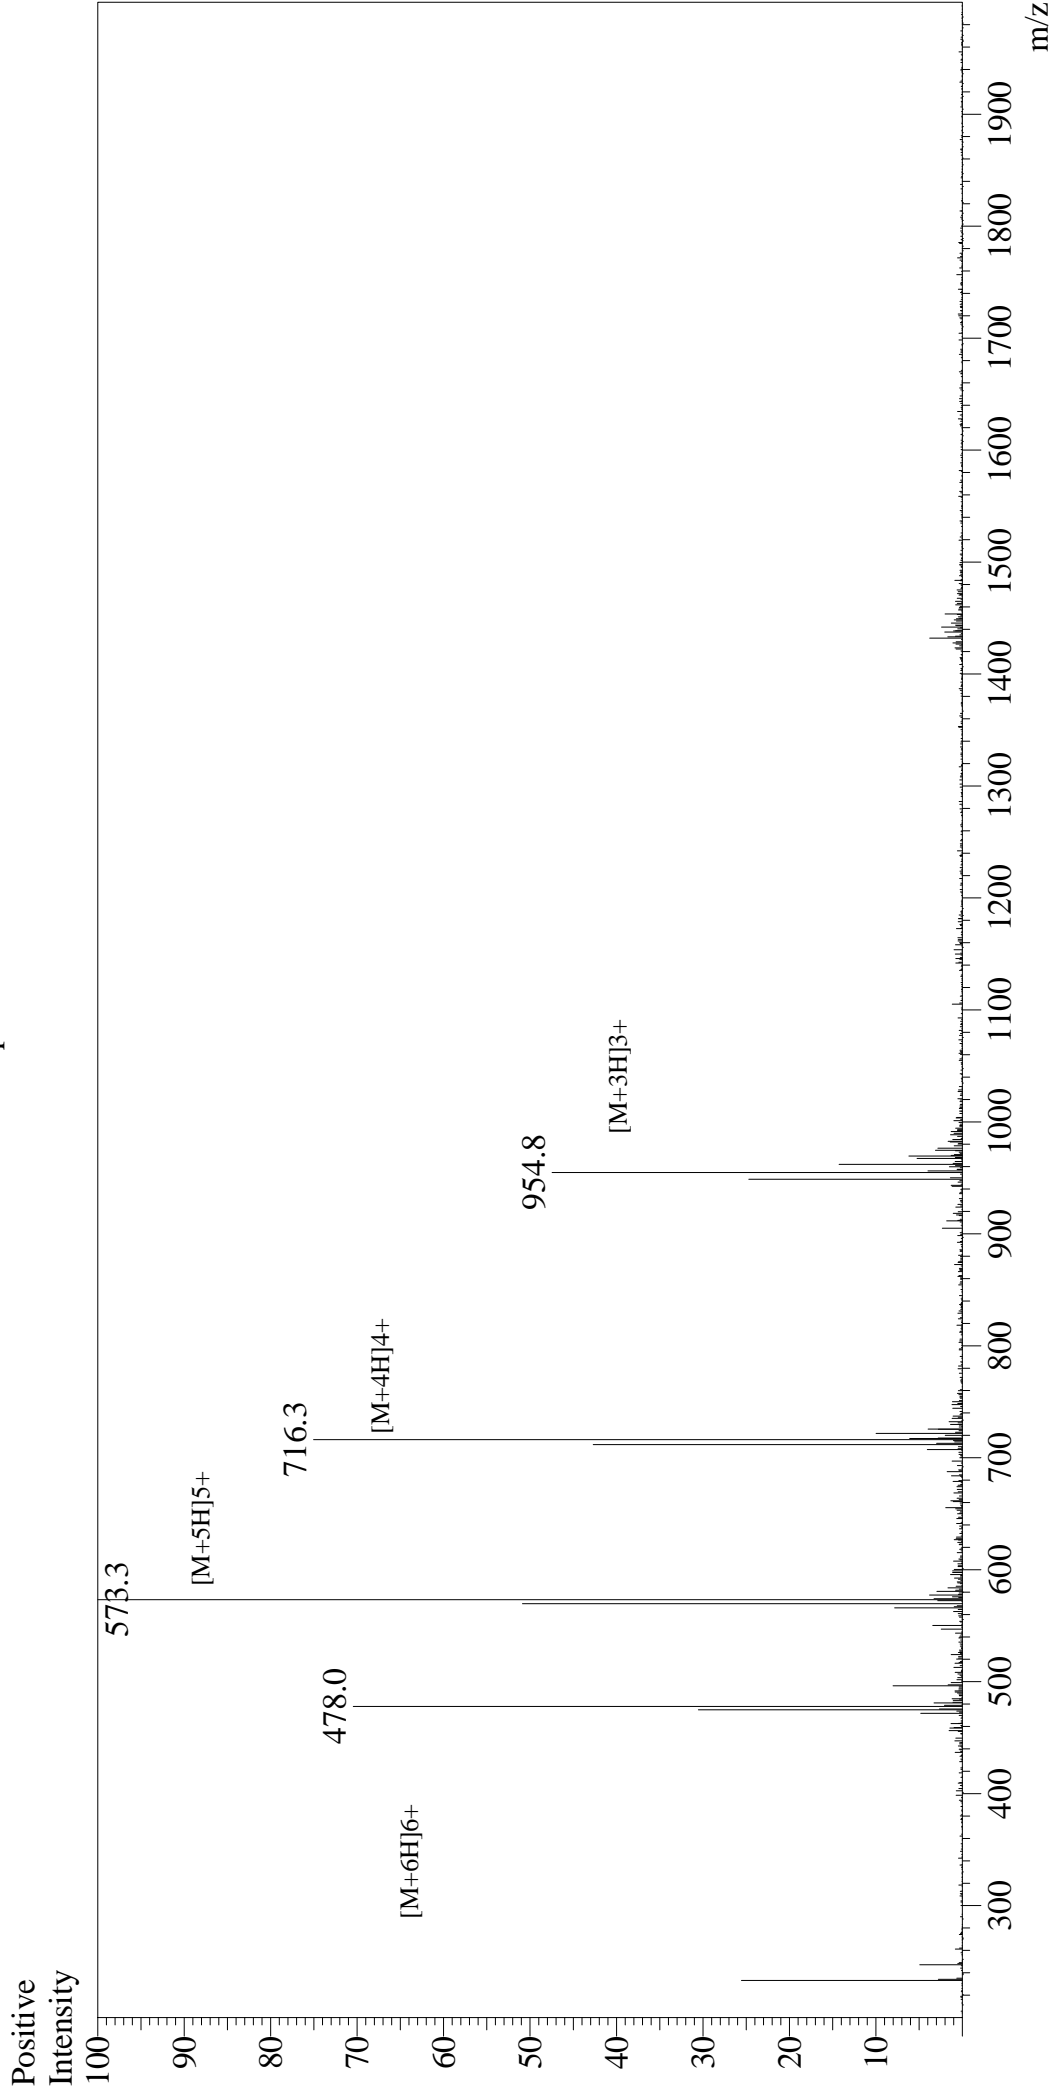

Sample Information

User : Gary
Month-Day Processed : 04/21/20
Time Processed : 8:16:44
Injection Volume : 0.3
Sample Name : MDYKDHGDYKDHIDYKDDDDK peptide
Cat No. : RP21087
Lot No. : E2230620D
Theoretical MW : 2861.87
Observed MW : 2861.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH