

Sample Name: β -Amyloid (1-42), human
 Cat. No. : RP20527
 Lot. No. : E0667721E
 Time Processed : 14:21:52
 Month-Day-Year Processed : 06/19/2021
 Pump A : 0.1% Ammonia solution in 100% water (v/v)
 Pump B : 0.1% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm
 Equipment : SS-CM-0309

<Chromatogram>

mV

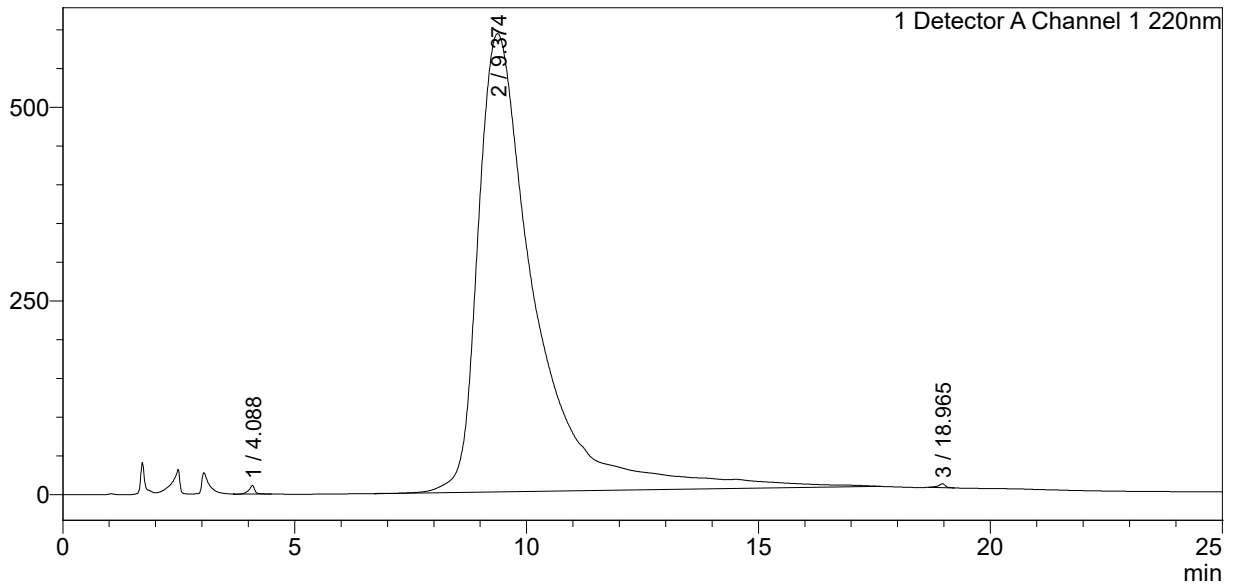

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.088	99028	11121	0.194
2	9.374	50911883	591189	99.706
3	18.965	51145	4979	0.100
Total		51062055	607289	100.000