

Sample Name : HA Peptide

Cat No. :RP11735 Lot No. : PE8791801

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

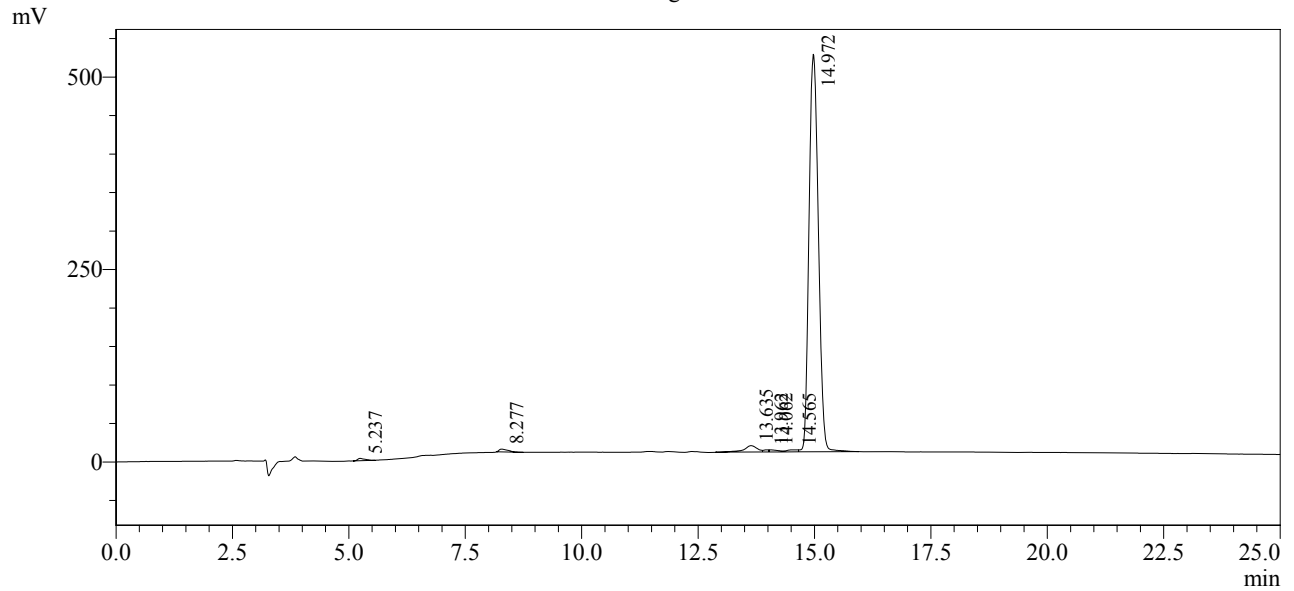

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.237	34413	3093	0.454
2	8.277	46175	3628	0.609
3	13.635	164126	8285	2.164
4	13.962	21663	2709	0.286
5	14.062	34707	2650	0.458
6	14.565	45365	2574	0.598
7	14.972	7236415	516373	95.431
Total		7582864	539311	100.000