

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. : RP21087
 Lot No. : E3662620J
 Time Processed : 7:27:16
 Month-Day-Year Processed : 11/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
37.00	Pumps	Pump B Conc.	95
37.01	Pumps	Pump B Conc.	5
42.00	Pumps	Pump B Conc.	5
42.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

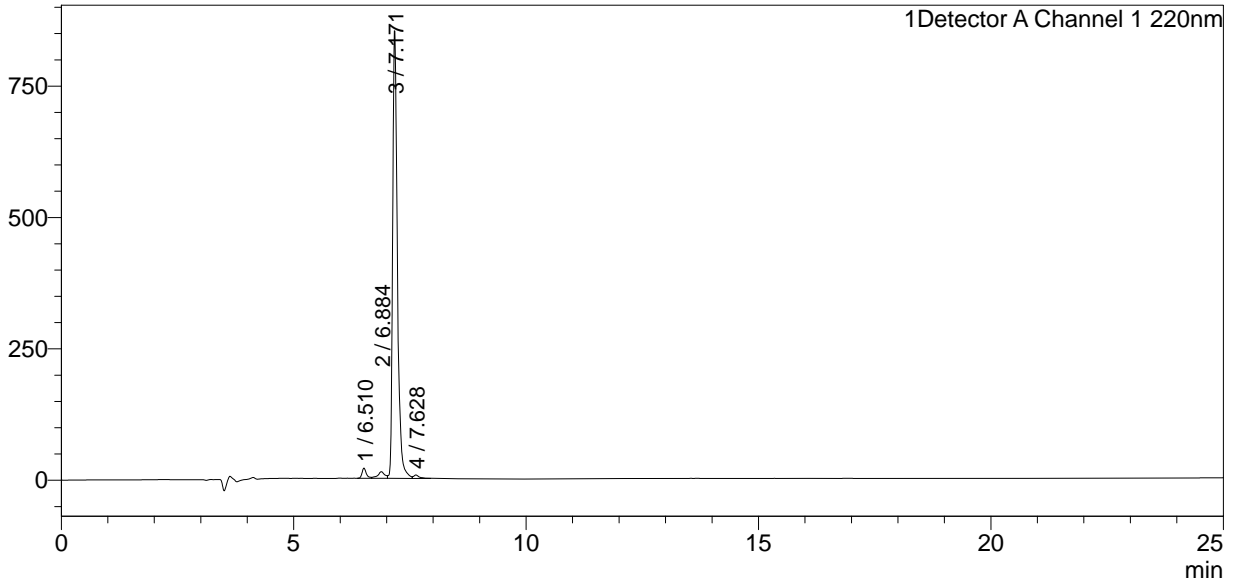

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.510	125487	19415	1.986
2	6.884	134198	12848	2.124
3	7.171	6003249	851637	95.020
4	7.628	54939	6619	0.870
Total		6317872	890518	100.000