

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E7293019L
 Time Processed : 15:57:20
 Month-Day-Year Processed : 12/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

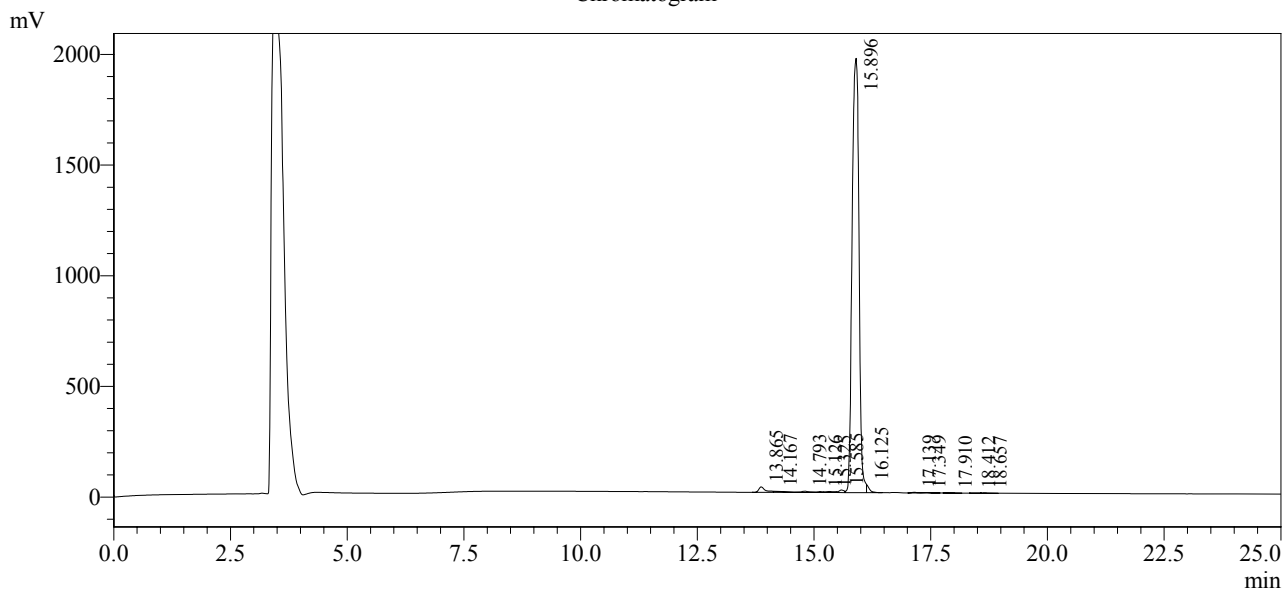

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.865	249468	25044	1.194
2	14.167	108218	5648	0.518
3	14.793	80135	5916	0.384
4	15.126	35210	4158	0.169
5	15.325	62521	4688	0.299
6	15.585	90075	11683	0.431
7	15.896	20067970	1962631	96.062
8	16.125	142822	37627	0.684
9	17.139	20332	3102	0.097
10	17.349	19846	2185	0.095
11	17.910	7168	768	0.034
12	18.412	1617	258	0.008
13	18.657	5261	838	0.025
Total		20890643	2064546	100.000