

Sample Name:C-Peptide (3-33), human  
 Cat No:RP11116  
 Lot No :E6364620L  
 Time Processed :11:40:22 AM  
 Month-Day-Year Processed :12/29/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.10	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
50.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

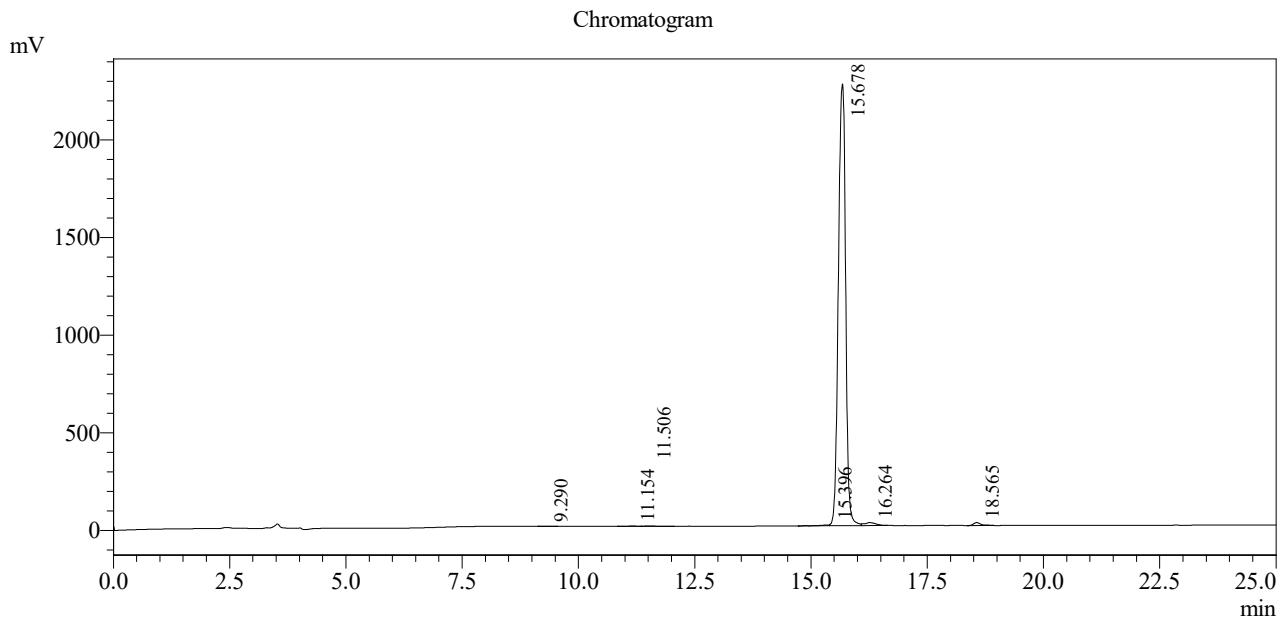

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.290	1482	207	0.006
2	11.154	5142	921	0.021
3	11.506	10086	1507	0.040
4	15.396	50463	4448	0.202
5	15.678	24511365	2261686	98.058
6	16.264	249262	15039	0.997
7	18.565	168938	15244	0.676
Total		24996737	2299053	100.000