

Sample Name : β -Amyloid (1-42), human
 Cat.No : RP10017
 Lot.No : E1999921A
 Time Processed: 19:47:50
 Year-Month-Day: 2021/1/15

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm


<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	10	
25.00	Pumps	Solvent B Conc.	100	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	10	
33.00	Pumps	Solvent B Conc.	10	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

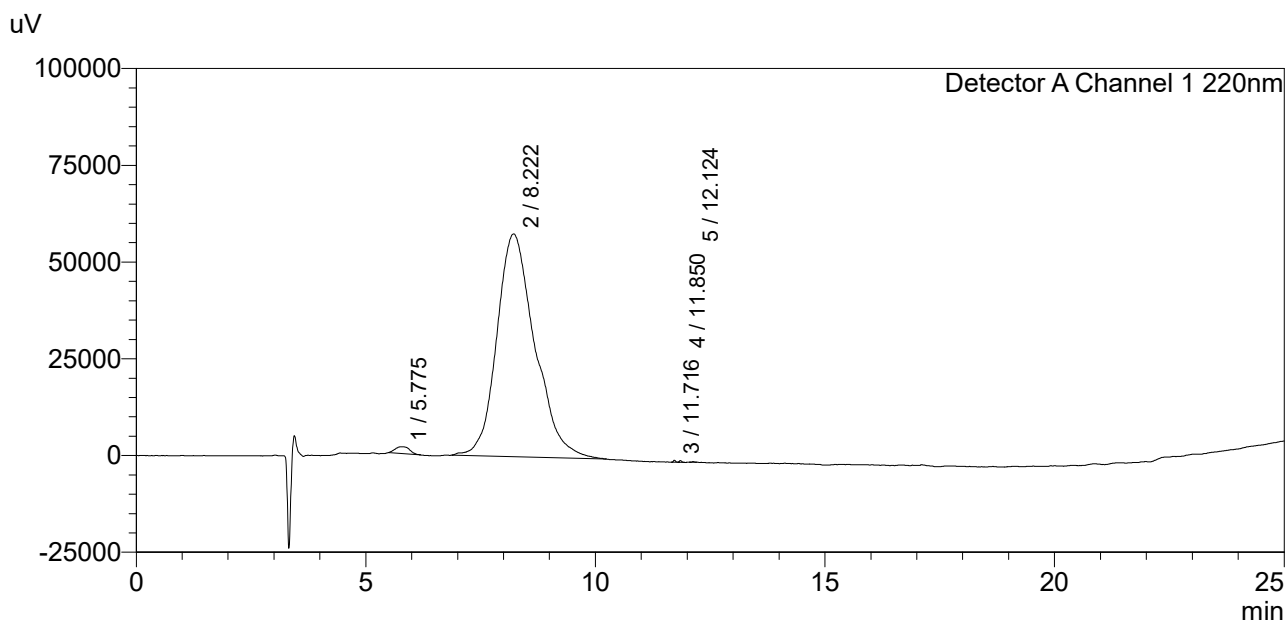

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.775	37221	1740	1.107
2	8.222	3320181	57601	98.776
3	11.716	1798	531	0.053
4	11.850	1566	461	0.047
5	12.124	551	169	0.016
Total		3361317	60501	100.000