

Sample Name :HA Peptide  
 Cat. No. :RP11735  
 Lot. No. :PE7201811  
 Time Processed :10:57:48  
 Month-Day-Year Processed :11/27/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

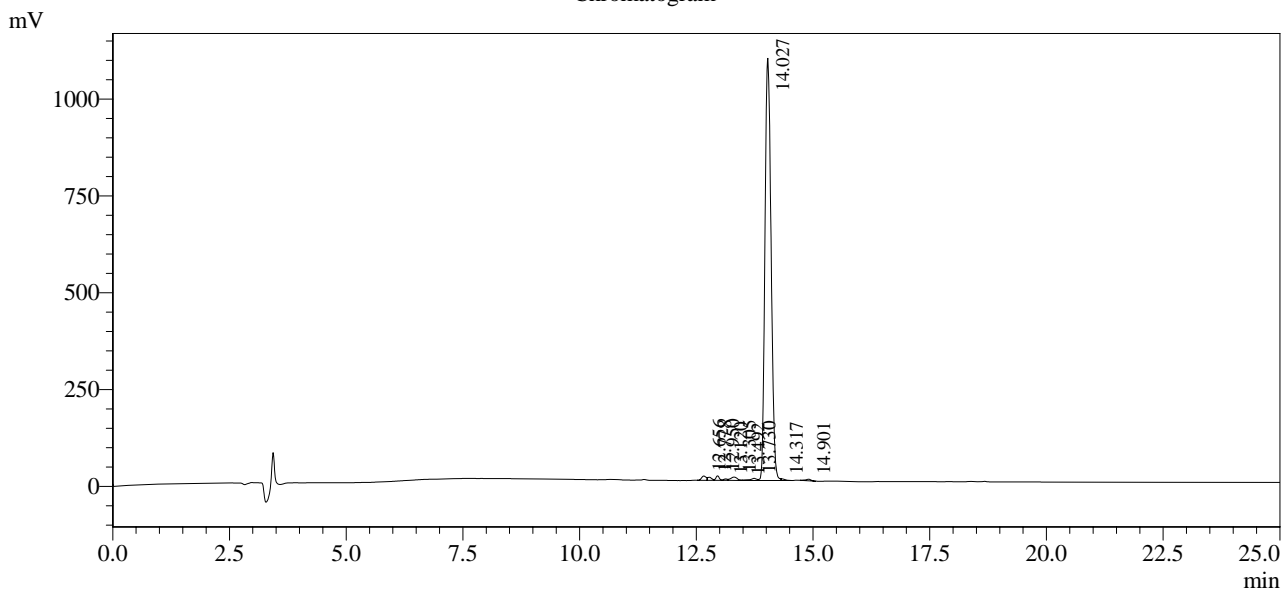

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.656	79164	11307	0.763
2	12.778	48426	8136	0.467
3	12.950	60352	11813	0.582
4	13.120	23496	3954	0.227
5	13.305	83989	8605	0.810
6	13.492	5448	1286	0.053
7	13.730	50201	5453	0.484
8	14.027	9968492	1090307	96.110
9	14.317	22103	4347	0.213
10	14.901	30291	4013	0.292
Total		10371963	1149221	100.000