

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E9412921D
 Time Processed :3:23:03 AM
 Month-Day-Year Processed :04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

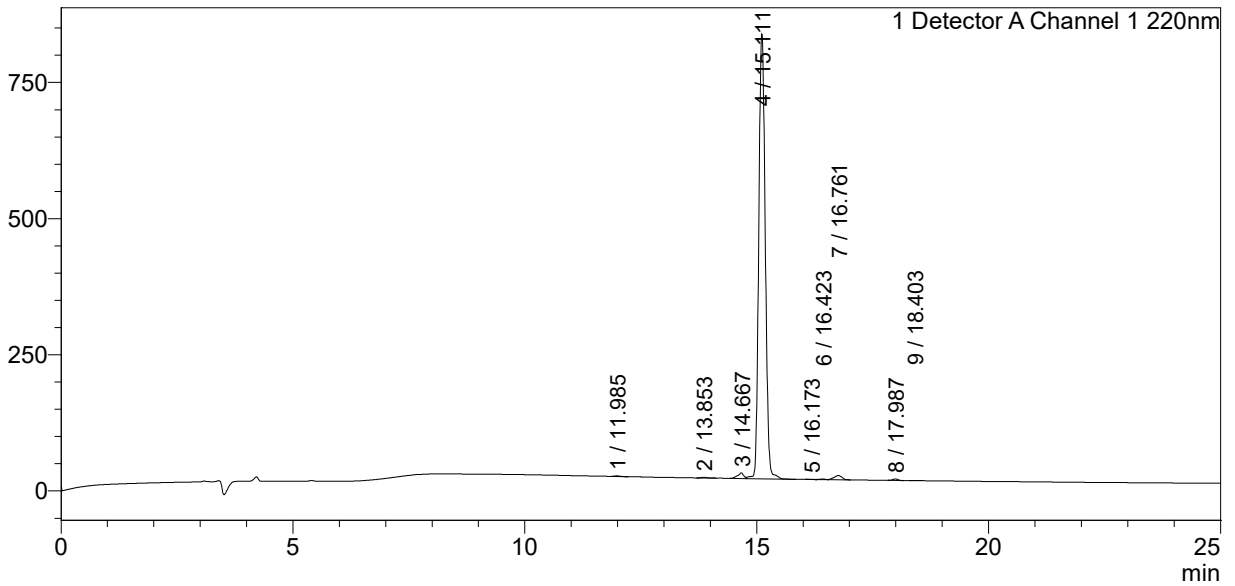

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.985	8097	1113	0.099
2	13.853	11127	1152	0.136
3	14.667	91758	10364	1.123
4	15.111	7944033	817442	97.187
5	16.173	2831	479	0.035
6	16.423	6626	868	0.081
7	16.761	86675	7602	1.060
8	17.987	20674	2653	0.253
9	18.403	2123	339	0.026
Total		8173945	842013	100.000