

Sample Name: β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E7118521D
 Time Processed: 8:15:36
 Month-Day-Year Processed :04/04/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

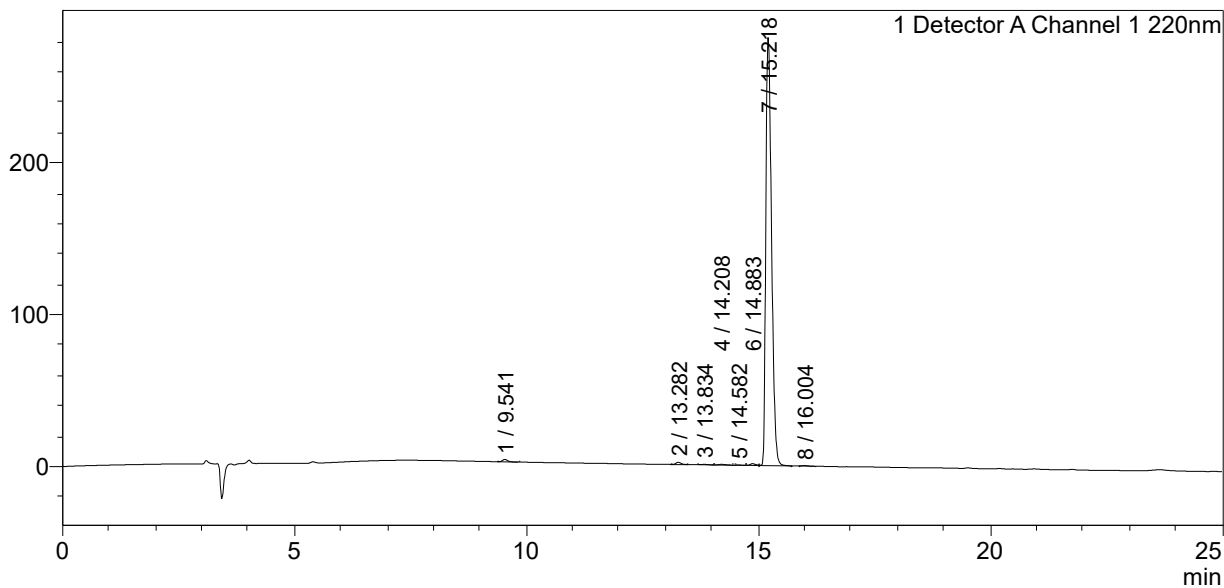

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.541	12592	1640	0.514
2	13.282	11465	1431	0.468
3	13.834	2095	248	0.085
4	14.208	4908	443	0.200
5	14.582	1059	167	0.043
6	14.883	9282	1100	0.379
7	15.218	2406997	282151	98.200
8	16.004	2714	374	0.111
Total		2451111	287554	100.000