

Sample Name :β-Amyloid (1-42), human  
 Cat No :RP10017  
 Lot No :E7746521B  
 Time Processed :3:19:56 PM  
 Month-Day-Year Processed :02/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	10
25.00	Pumps	Pump A B.Conc	100
27.00	Pumps	Pump A B.Conc	100
27.01	Pumps	Pump A B.Conc	10
35.00	Pumps	Pump A B.Conc	10
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010011

<Chromatogram>

mV

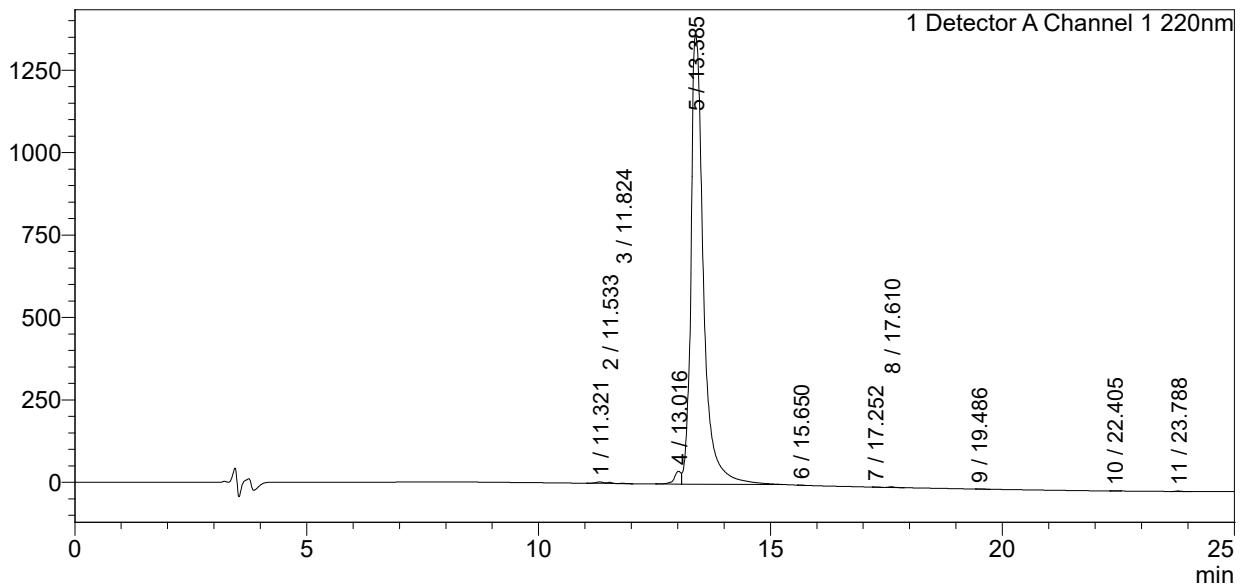

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.321	45339	4197	0.174
2	11.533	20832	3335	0.080
3	11.824	5506	678	0.021
4	13.016	396613	38857	1.519
5	13.385	25610112	1360258	98.060
6	15.650	3234	644	0.012
7	17.252	1558	237	0.006
8	17.610	15071	2439	0.058
9	19.486	5012	620	0.019
10	22.405	1730	315	0.007
11	23.788	11755	1381	0.045
Total		26116762	1412959	100.000