

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No: RP21087
 Lot No : E0967921H
 Time Processed :9:15:19
 Month-Day-Year Processed :08/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

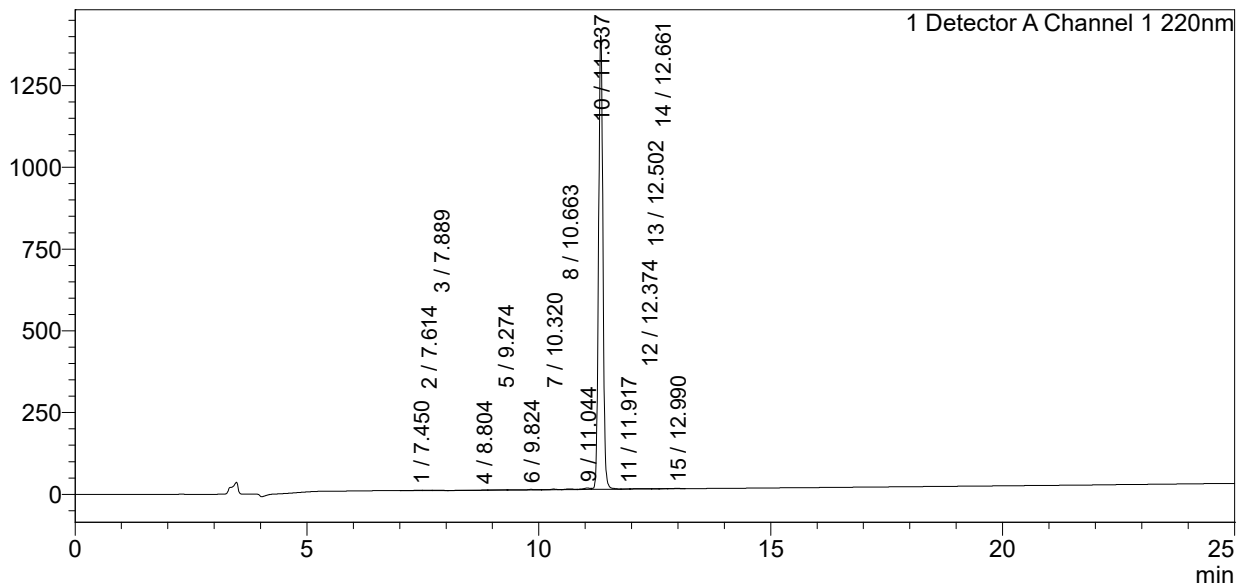

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.450	9205	547	0.099
2	7.614	7816	640	0.084
3	7.889	10433	749	0.113
4	8.804	18567	537	0.200
5	9.274	7601	269	0.082
6	9.824	18547	1520	0.200
7	10.320	17550	1893	0.189
8	10.663	24773	2137	0.267
9	11.044	49558	4721	0.535
10	11.337	9040551	1387831	97.536
11	11.917	9205	845	0.099
12	12.374	25701	1188	0.277
13	12.502	8807	1084	0.095
14	12.661	6284	734	0.068
15	12.990	14311	1303	0.154
Total		9268909	1405998	100.000