

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E7370720A
 Time Processed : 7:02:58
 Month-Day-Year Processed : 01/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

Chromatogram

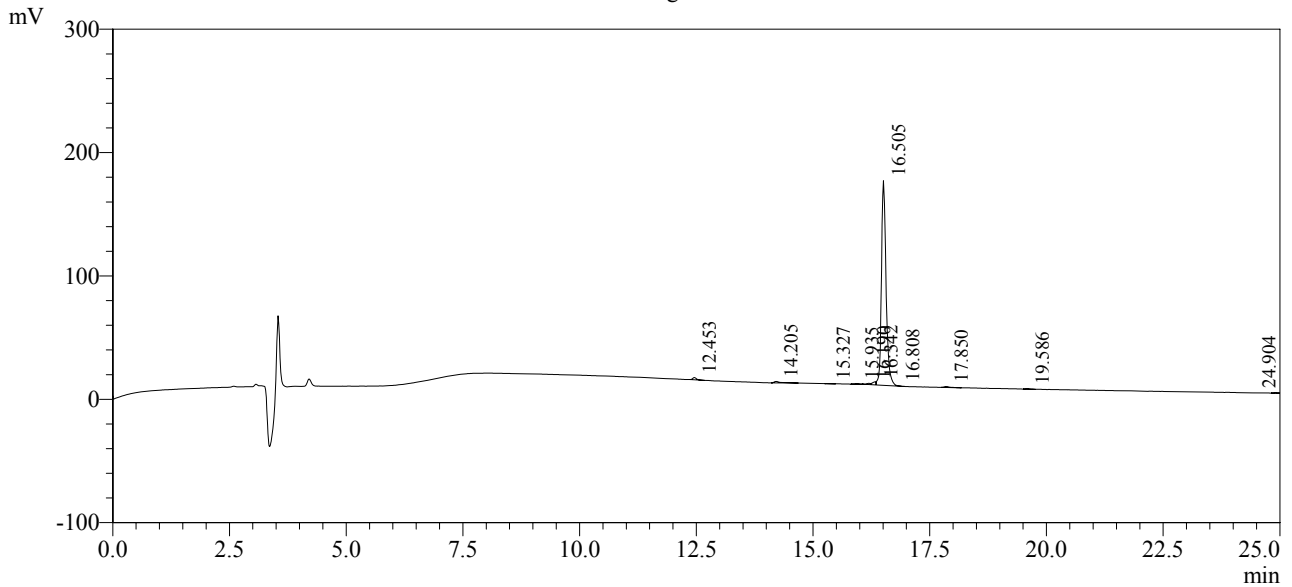

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.453	10081	1816	0.840
2	14.205	10255	1174	0.855
3	15.327	1126	192	0.094
4	15.935	2170	304	0.181
5	16.190	5419	947	0.452
6	16.342	13258	2472	1.105
7	16.505	1146982	165895	95.599
8	16.808	1478	403	0.123
9	17.850	6158	775	0.513
10	19.586	1717	268	0.143
11	24.904	1139	196	0.095
Total		1199781	174440	100.000